

Award Number: W81XWH-12-2-0111

TITLE: Deployment Ready Airway Management System (DRAMS)

PRINCIPAL INVESTIGATOR: Richard B. Schwartz, MD

CONTRACTING ORGANIZATION: AI Medical Devices, Inc.
Evans, GA 30809-5471

REPORT DATE: October 2013

TYPE OF REPORT: Annual

PREPARED FOR: U.S. Army Medical Research and Materiel Command
Fort Detrick, Maryland 21702-5012

DISTRIBUTION STATEMENT: Approved for Public Release;
Distribution Unlimited

The views, opinions and/or findings contained in this report are those of the author(s) and should not be construed as an official Department of the Army position, policy or decision unless so designated by other documentation.

REPORT DOCUMENTATION PAGE				Form Approved OMB No. 0704-0188	
Public reporting burden for this collection of information is estimated to average 1 hour per response, including the time for reviewing instructions, searching existing data sources, gathering and maintaining the data needed, and completing and reviewing this collection of information. Send comments regarding this burden estimate or any other aspect of this collection of information, including suggestions for reducing this burden to Department of Defense, Washington Headquarters Services, Directorate for Information Operations and Reports (0704-0188), 1215 Jefferson Davis Highway, Suite 1204, Arlington, VA 22202-4302. Respondents should be aware that notwithstanding any other provision of law, no person shall be subject to any penalty for failing to comply with a collection of information if it does not display a currently valid OMB control number. PLEASE DO NOT RETURN YOUR FORM TO THE ABOVE ADDRESS.					
1. REPORT DATE October 2013		2. REPORT TYPE Annual		3. DATES COVERED 28September2012 -27September2013	
4. TITLE AND SUBTITLE Deployment Ready Airway Management System (DRAMS)				5a. CONTRACT NUMBER	
				5b. GRANT NUMBER W81XWH-12-2-0111	
				5c. PROGRAM ELEMENT NUMBER	
6. AUTHOR(S) Richard B. Schwartz, MD email: rschwartz@gru.edu				5d. PROJECT NUMBER	
				5e. TASK NUMBER	
				5f. WORK UNIT NUMBER	
7. PERFORMING ORGANIZATION NAME(S) AND ADDRESS(ES) AI Medical Devices, Inc. Evans, GA 30809-5471				8. PERFORMING ORGANIZATION REPORT NUMBER	
9. SPONSORING / MONITORING AGENCY NAME(S) AND ADDRESS(ES) U.S. Army Medical Research and Materiel Command Fort Detrick, Maryland 21702-5012				10. SPONSOR/MONITOR'S ACRONYM(S)	
				11. SPONSOR/MONITOR'S REPORT NUMBER(S)	
12. DISTRIBUTION / AVAILABILITY STATEMENT Approved for Public Release; Distribution Unlimited					
13. SUPPLEMENTARY NOTES					
14. ABSTRACT Overall the project has progressed with excellent results. Alpha one and two prototypes have been developed and the initial Beta one prototype device manufactured. Civilian and Military airway experts have evaluated the B-1 prototype with excellent feedback. Minor modifications are being integrated into the prototype for completion of environmental and electrical safety testing. The B-1 Prototype will be utilized for initial clinical trials utilizing airway simulators in a difficult airway model.					
15. SUBJECT TERMS- none provided					
16. SECURITY CLASSIFICATION OF:			17. LIMITATION OF ABSTRACT UU	18. NUMBER OF PAGES 9	19a. NAME OF RESPONSIBLE PERSON USAMRMC
a. REPORT U	b. ABSTRACT U	c. THIS PAGE U			19b. TELEPHONE NUMBER (include area code)

AI Medical Devices

Annual Report

Award Number:	W81XWH-12-2-0111
Proposal Number:	11160001
Title:	Deployment Ready Airway Management System (DRAMS)
PI Name:	Richard B. Schwartz, MD
PI Organization and Address:	AI Medical Devices, Inc. 4403 Ferry Landing Evans, GA 30809-5471
PI Phone and Email:	(706) 533-2942 rschwartz@gru.edu
Report Date:	10-24-13
Report Period:	Sept. 2012 – Oct. 2013
Contracting or Grants Officer's Representative:	Maribel Fratina




Project Summary:

Overall the project has progressed with excellent results. Alpha one and two prototypes have been developed and the initial Beta one prototype device manufactured. Civilian and Military airway experts have evaluated the B-1 prototype with excellent feedback. Minor modifications are being integrated into the prototype for completion of environmental and electrical safety testing. The B-1 Prototype will be utilized for initial clinical trials utilizing airway simulators in a difficult airway model.

Project Accomplishments:

The following milestones have been completed as listed in the proposal:

1. Handle and Monitor Housing Development: The project has gone through the use of multiple evolutions of 3D models and the use of rapid prototyping culminating in the B-1 prototype that has meet with excellent feedback from airway experts.

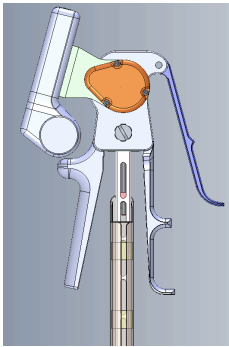

A hand is holding a blue manual sphygmomanometer. The device features a clear circular pressure gauge with a needle, a blue inflation bulb, and a black inflatable cuff. A black tube connects the cuff to the gauge. The background is a plain, light-colored surface.


Disposable sheath prototype development.

Multiple versions of disposable sheath prototypes have been developed culminating in the B-1 prototype with excellent video transmission and functional results.

Alpha 1 and Alpha 2 prototypes



3D Models of B-1 Prototype

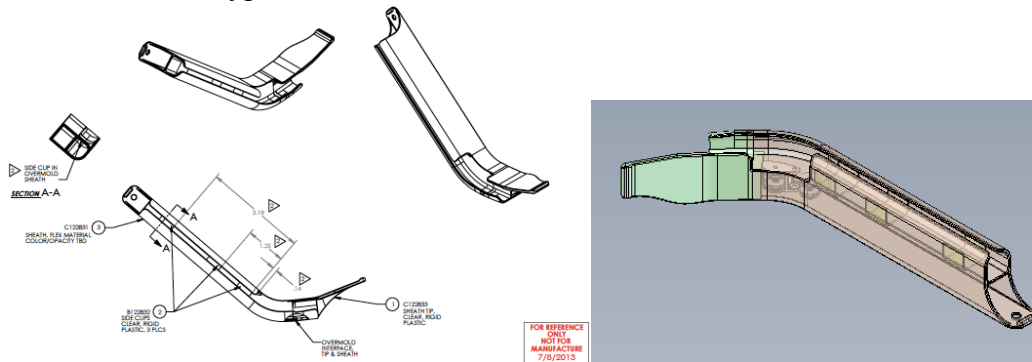

B-1 Disposable Sheath




Video Image Through the Disposable Sheath



FlexBlade Working Length Development:

Several versions of the working length have been developed along with rapid prototypes. The results have been excellent and DMLS Alpha one and two prototypes have been developed resulting in a B-1 prototype. Several evolutions of waterproof contacts have been developed with a B-1 prototype developed.

SLA of Electrical Contact Model

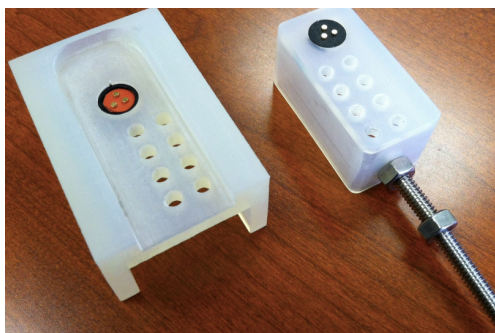

DMLS FlexBlade Reusable Module B-1 Prototype



Completed B-1 Prototypes:

B-1 Articulated with ET Tube

B-1 Relaxed with ET Tube





Relaxed in Simulator

Flexed in Simulator

Tube Advanced

Clinical Studies: The B-1 prototypes have meet all required feedback from airway experts and the device is ready to begin trials in Cadavers and the initial clinical trial in simulators. Protocols should be submitted to the IRB in Nov. 2013.

Project Progress: The project has made substantial progress and has resulted in an excellent B-1 prototype that will be used in clinical trials. The final environmental testing and electrical safety testing should be completed in the next quarter.

Barriers Encountered: The project experienced some upfront delay as all original quotes from the proposal had expired before final funding had been procured. Substantial delays in reimbursement for the project has lead to frequent delays in the project. Despite these barriers we should be able to complete the project on time.

Budget/Financial Report:

	Cumulative
Personnel	\$61,999.04
Fringe Benefits	0
Travel	\$1,537.72
Equipment	0
Supplies	\$7,511.70
Other	0
Subaward - Organization	\$214,656.56
Subtotal	\$285,705.02
Indirect Costs	0
Fees	0
TOTAL	\$285,705.02